


+ technical operation



+ optional

- Integrated barcode reader to read the serial number of endoscopes and operators and related traceability of the executed cycles downloading data from USB port (already equipped with 50 instrument acid-resistant barcode labels and 20 for operators).
- Olympus, Pentax, Fujinon and Storz leak test connectors.

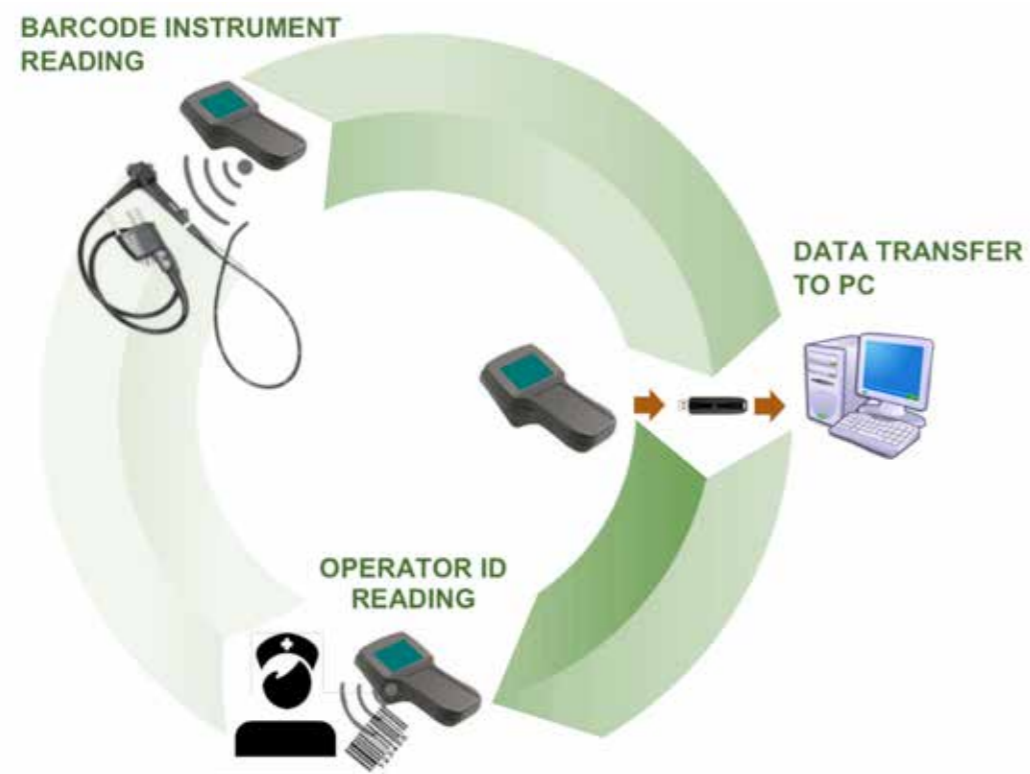

**MEDICAL DEVICES GROUP Srl**  
 Via G.Fracastoro, 1 48124 Ravenna (RA)  
 Tel +39 0544 1826013  
 Fax +39 0544 1826015  
 www.mdg-srl.com - info@mdg-srl.com



Complies with the Directive 93/42/CEE Annex VII

# LT-217<sup>®</sup>

tester to check integrity of flexible endoscopes

+  
 For all types of flexible endoscopes  
 mdg - patent

giantucalerrini.com  
 Vers. 1/2018



**DATA TRANSFER**  
through USB flash drive



**DISPLAY LCD**  
backlit LCD display



**CONNECTORS**

Instrument connectors for each brand



**AUTOMATIC RECOGNITION**  
it recognizes automatically the instrument



**INTERGRATED BAR CODE**  
to read operator an instrument ID



Italian  
technology  
and design



**LT-217®**  
To check endoscope  
channels, sheaths  
and o'ring conditions



# LT-217®

tester to check integrity of flexible  
endoscopes

**LT-217®** is a patented system designed to check the integrity of flexible endoscopes. The device detects accurately leakage of the sheaths, of the endoscopes channels and the wear conditions of the o'ring.

It checks also the conditions of internal channels and the little holes caused by twisted biopsy channels. This leak tester works through much higher standard compared to the actual product on the market and because of this it drastically reduces infiltrations during endoscope reprocessing procedures.

**LT-217®** is a MDG s.r.l. patent.

**Standard equipment:**

- Power supply for internal batteries
- Connection hose
- Leak test connector
- End-user and maintenance manual
- Flash drive cable to download the stored cycles.